

Robert E. Means Jr. M.D.

application number:

confirmation number:

docket number:

contact number: 443 5707190

410 4662496

screw driver attachment head

Slipped Capital Femoral Epiphysis Fixation Screw

outside diameter cutting 1/2
inside diam. < thread

fixation head

inside diam.


two full fixation threads

8mm. max. thread length

4.5mm. and 6.0mm.

outside diameter sizes


2mm max
thread height

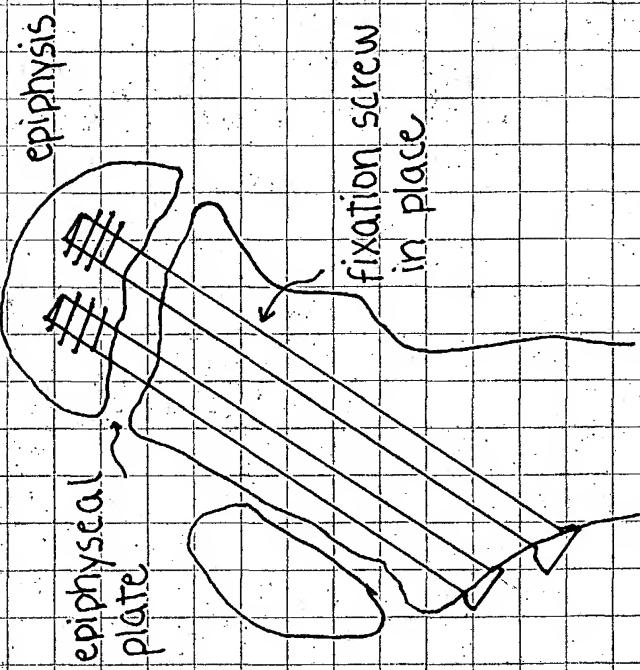

femoral head neck and intertrochanter region

FIG. 3.

FIG. 1.

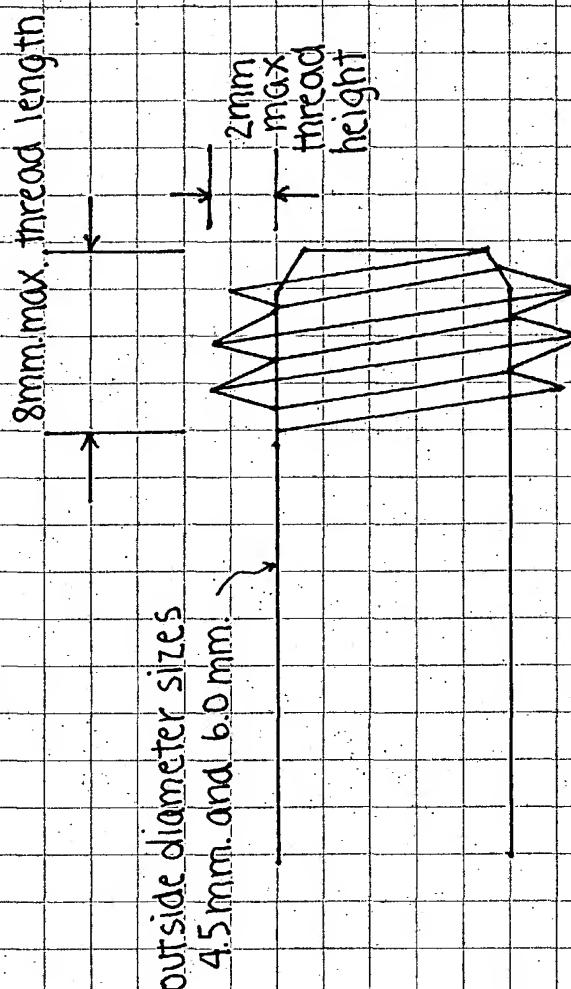

enlarged view

FIG. 2.